


Diethylene Glycol and Diols

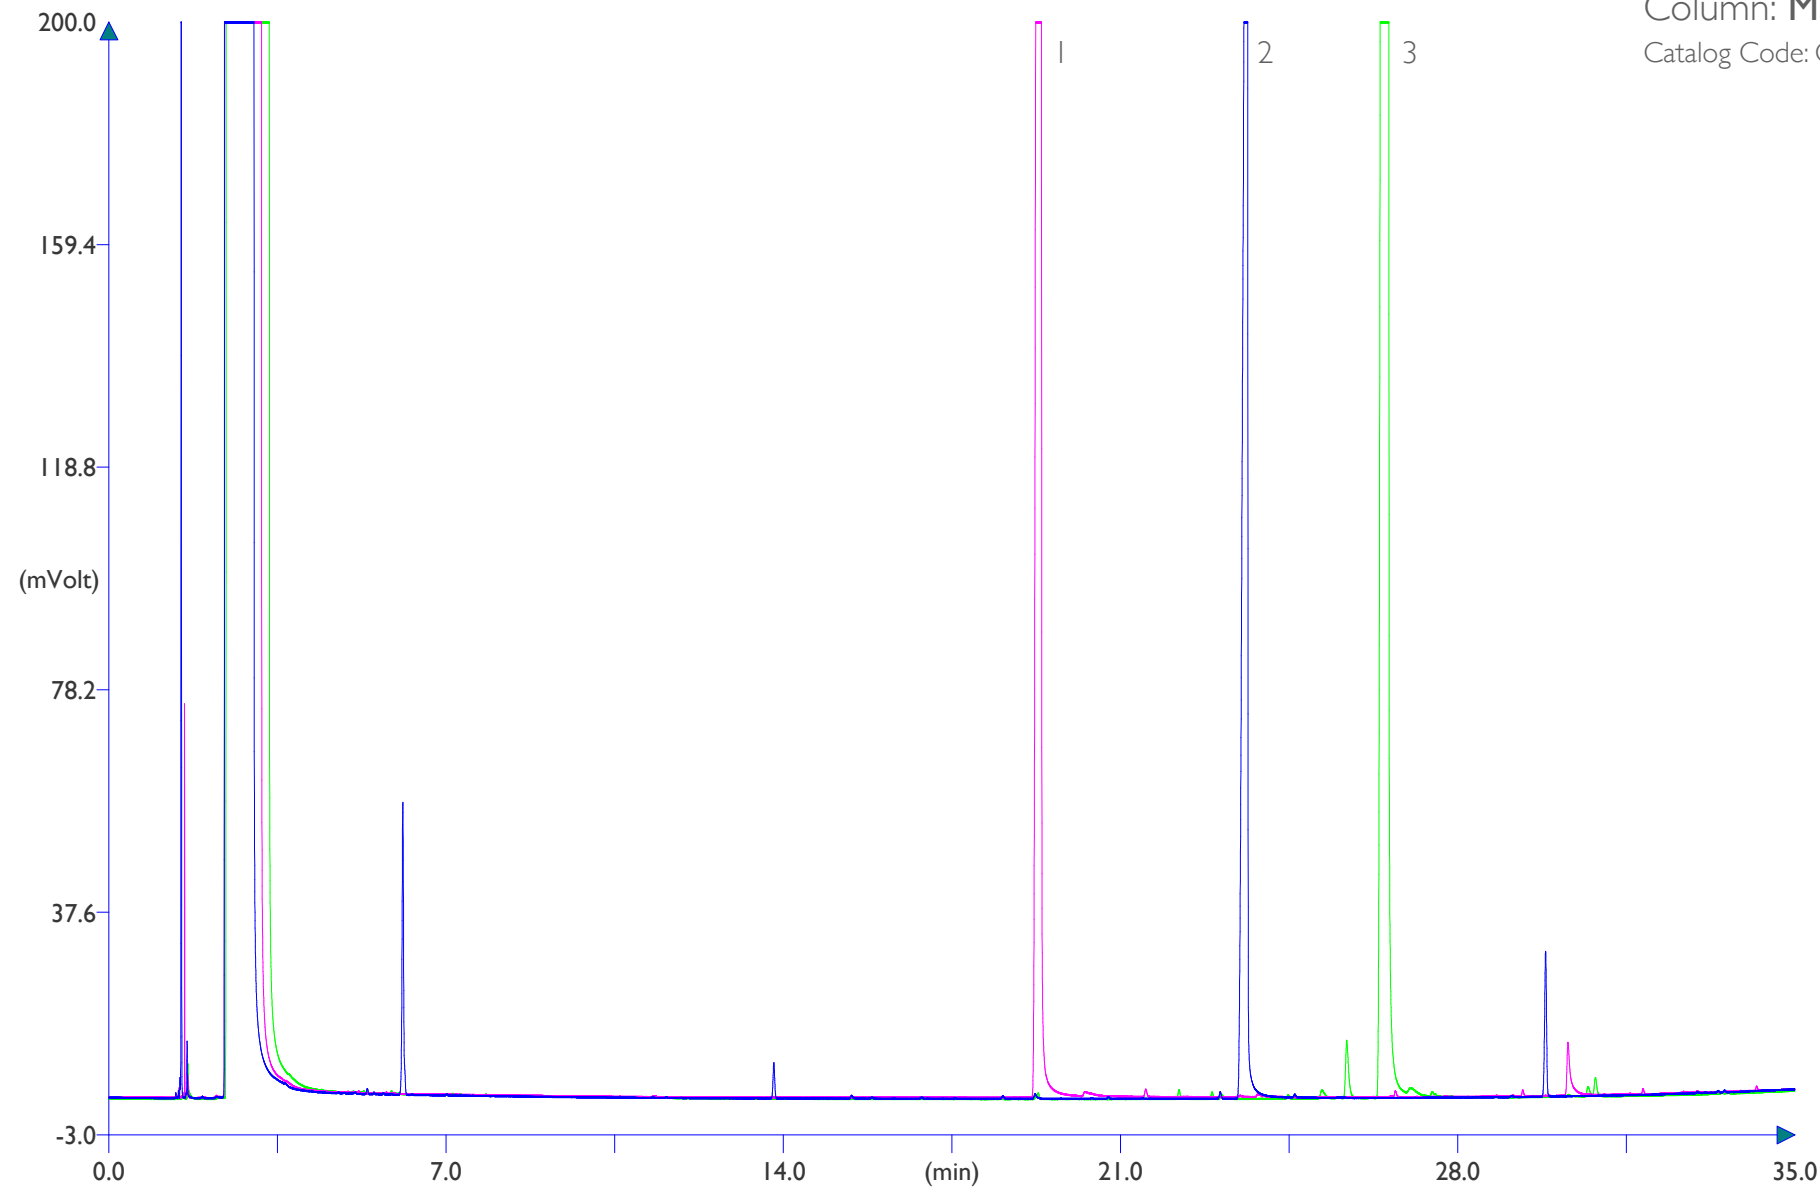

Column: **MEGA-ACID (FFAP)** - 0.32mm, 0.50 μ m, 50m
Catalog Code: C-ACID-032-050-50

Conditions:

Injection: Split, 250°C, 50mL/min split flow,
1 μ L injected volume, 0.2% each compound sample
dilution.

Detector: FID 250°C.

Oven Program: 65°C, 5°C/min, 245°C.

Carrier Gas: Hydrogen, 100kPa.

1. 1,2-Pentenediol
2. Diethylene Glycol
3. 1,2-Octenediol



since
1980



contact us: info@mega.mi.it

 follow us [@MEGAColumns](https://twitter.com/MEGAColumns)

www.mega.mi.it