


Benzene and aromatic volatile compounds in air

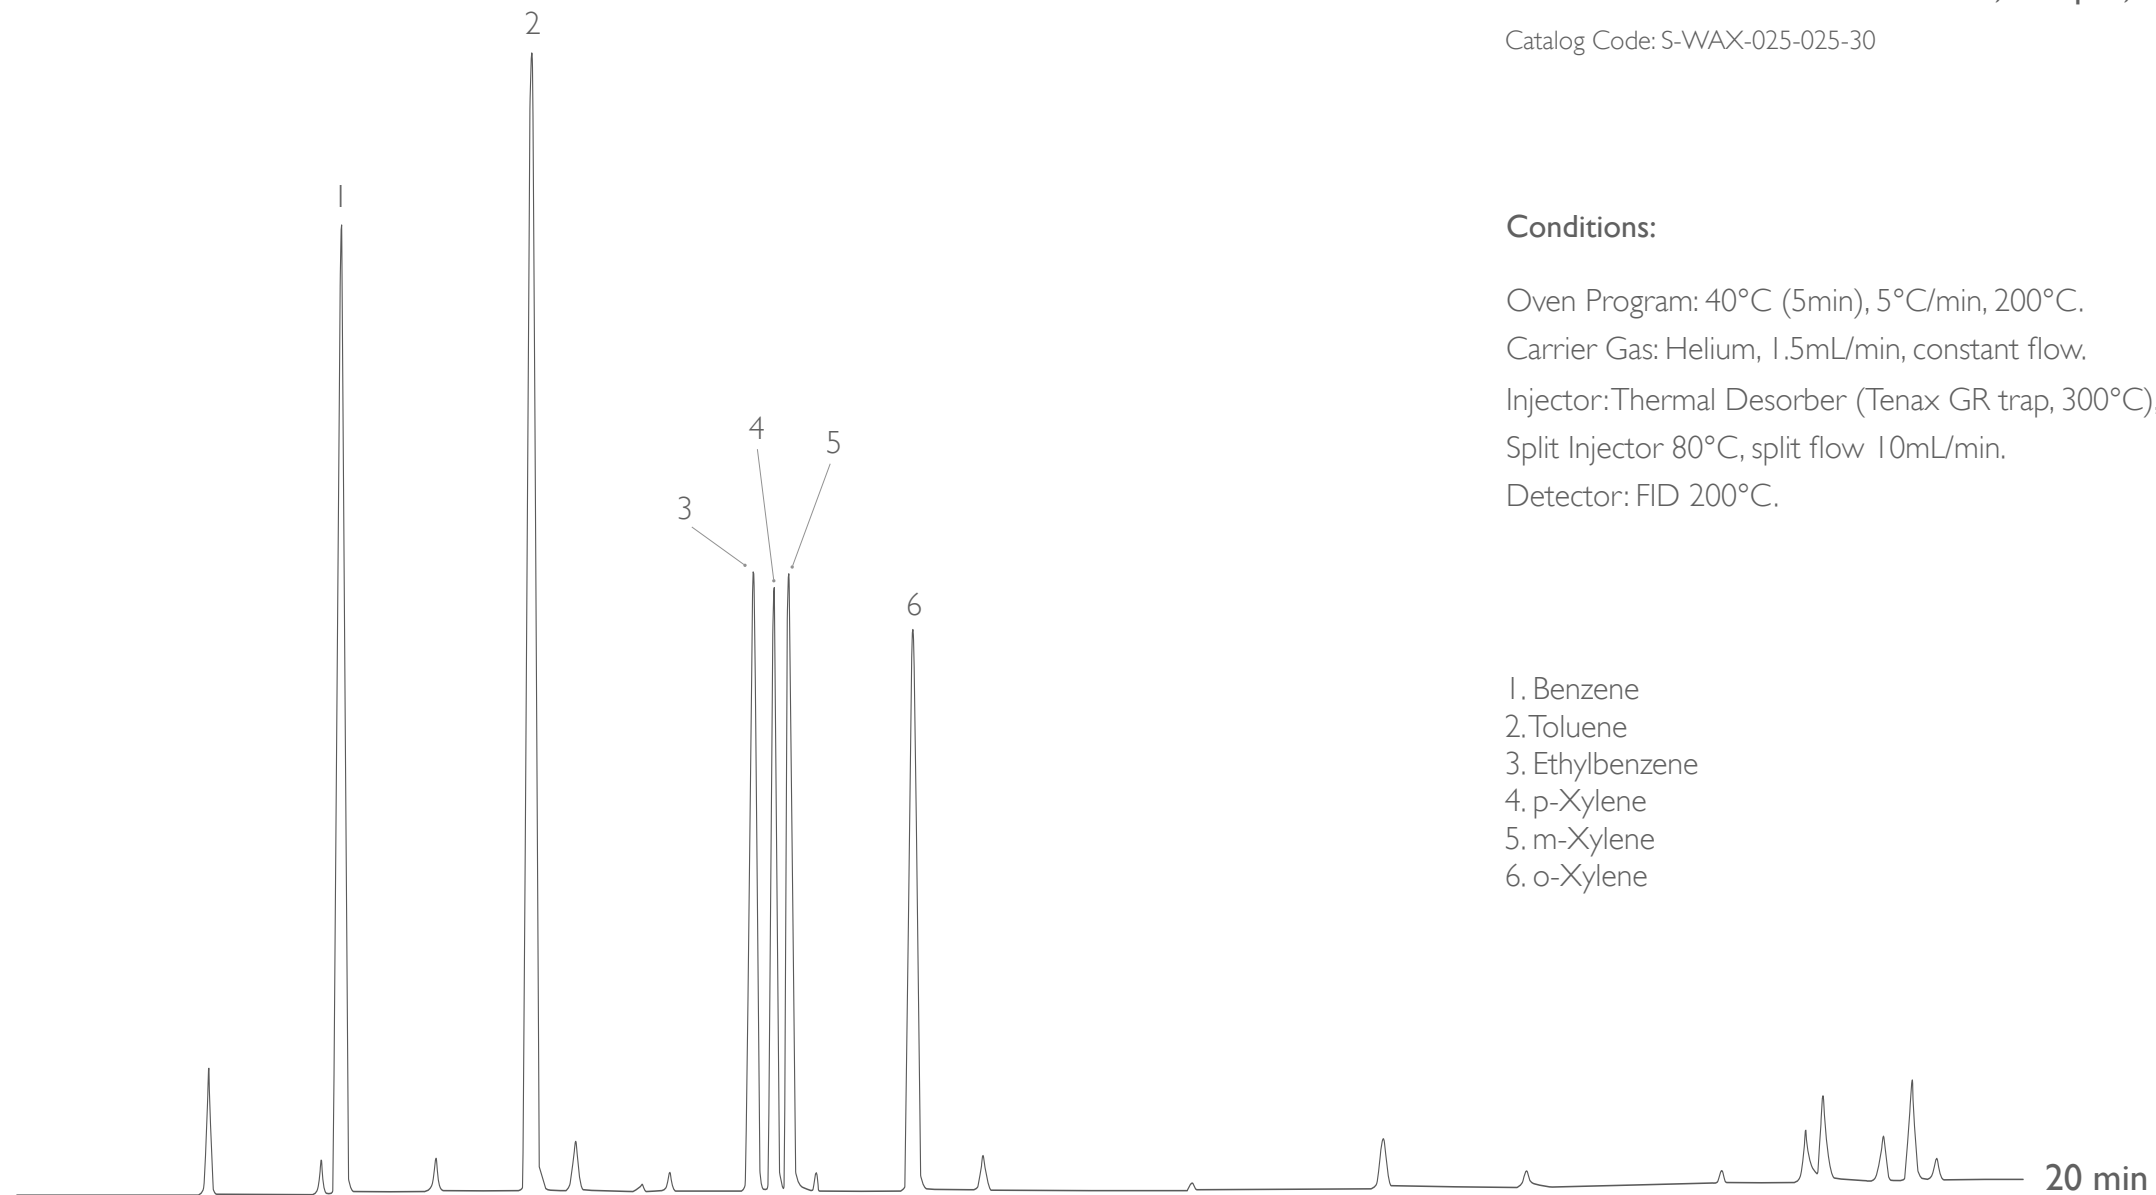

Analysis carried out with DANI Master GC.

Column: **MEGA-WAX** - 0.25mm, 0.25 μ m, 30m

Catalog Code: S-WAX-025-025-30

Conditions:

Oven Program: 40°C (5min), 5°C/min, 200°C.

Carrier Gas: Helium, 1.5mL/min, constant flow.

Injector: Thermal Desorber (Tenax GR trap, 300°C),

Split Injector 80°C, split flow 10mL/min.

Detector: FID 200°C.

1. Benzene
2. Toluene
3. Ethylbenzene
4. p-Xylene
5. m-Xylene
6. o-Xylene

MEGA[®]

www.mega.mi.it